


## DIGITAL INDICATOR --- Circuit Diagram

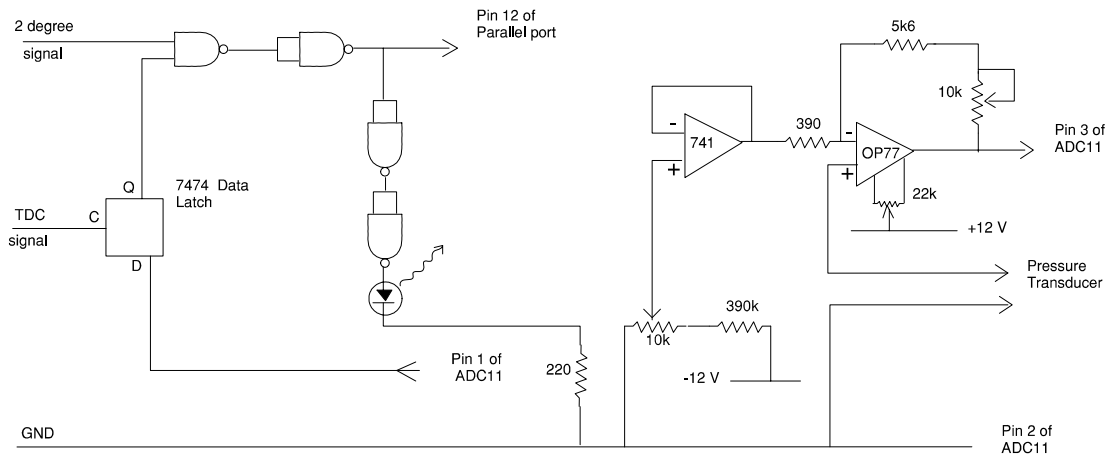

**NOTE:**

Power supplies (5V for digital chips, and +/- 12V for Op-amps) not shown.

The 741 follower is used to balance the offset voltage with Sensym transducers.

A separate power supply ( battery driven ) is required for the pressure transducer.  
(I use a 12V battery and a Ref01 regulator ( 10V ) )

The 5 & 12 volt supplies are extracted from the PC (the 5V supply also powers the opto-switches on the slotted disc)

W B H 2/97

## DIGITAL INDICATOR (PC version)

W B H 2/97

